

Flow Laboratory Traceability Chart/Capability

National Metrology
Institute




Working Standard
Calibration Laboratory



PRIMARY GAS FLOWMETER
A.P. BUCK MODEL M-5 ACCURACY $\pm 0.5\%$ RDG.


FLOW CALIBRATOR
OMEGA MODEL FTB-105, FTB-109
ACCURACY $\pm 1\%$ RDG.

Flow Instrument

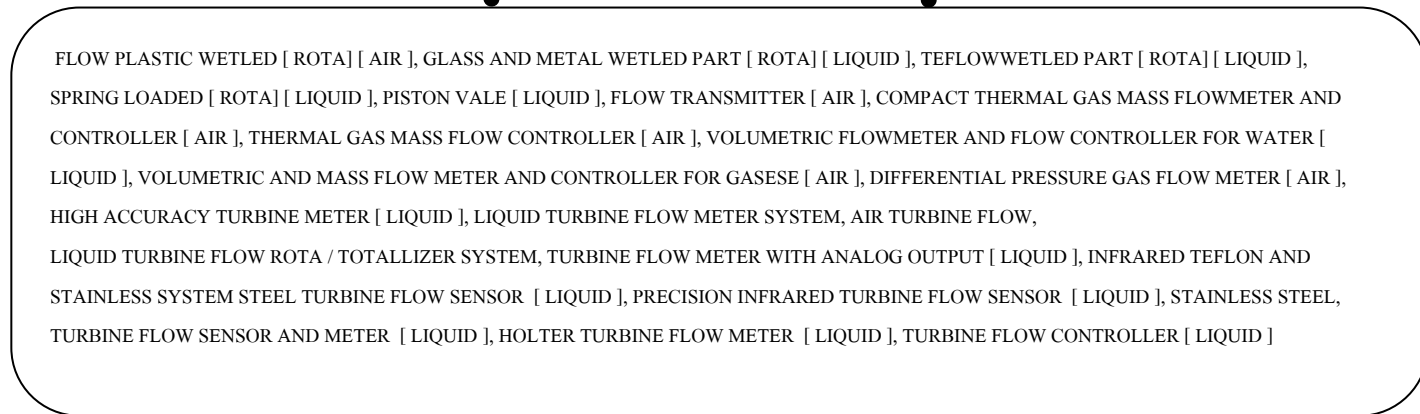


Flow Laboratory Traceability Chart/Capability

National Metrology
Institute



Working Standard
Calibration Laboratory



ULTRA FLOW METER
DYNASONIC MODEL DTFXP-B16A-NN
ACCURACY $\pm 0.5\%$ RDG.

Flow Instrument

