


Mass Laboratory Traceability Chart

National Metrology
Institute

Working Standard
Calibration Laboratory

Mass Instrument

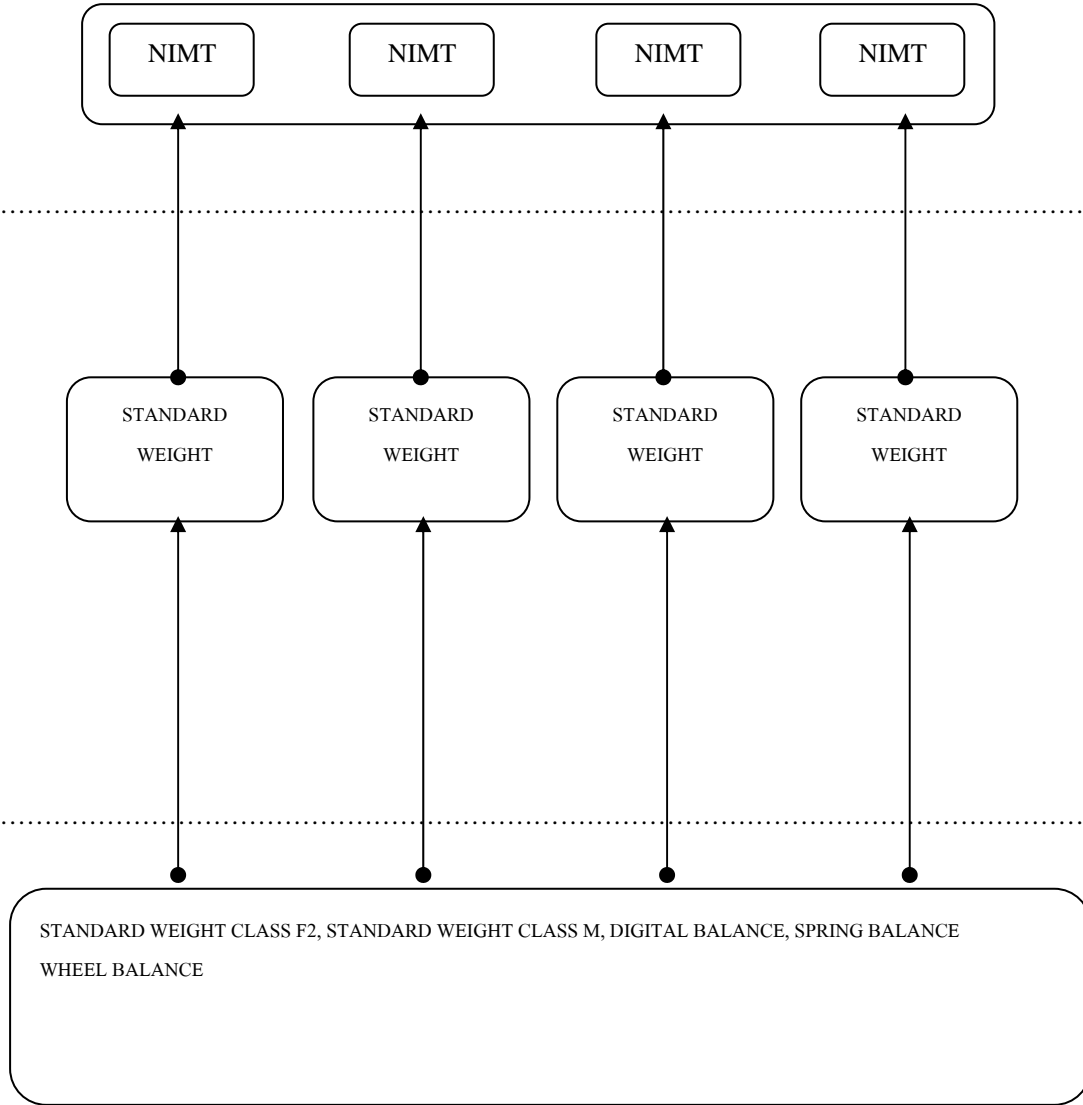

STANDARD WEIGHT
METTLER TOLEDO MODEL CLASS F1 ACCURACY CLASS F1


STANDARD WEIGHT
METTLER TOLEDO MODEL CLASS E2 ACCURACY CLASS E2

STANDARD WEIGHT
PD MODEL CLASS F2 ACCURACY CLASS F2



STANDARD WEIGHT
CLC MODEL CLASS M1 ACCURACY CLASS M1

Mass Laboratory Traceability Chart

National Metrology
Institute

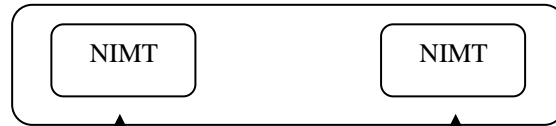

Working Standard
Calibration Laboratory



STANDARD WEIGHT
METTLER TOLEDO MODEL CLASS F1 ACCURACY CLASS F1

ELECTRONIC BALANCE
METTLER TOLEDO MODEL PR8002 ACCURACY ± 0.01 g

Mass Instrument

