



Vibration Laboratory Traceability Chart/Capability

National Metrology
Institute

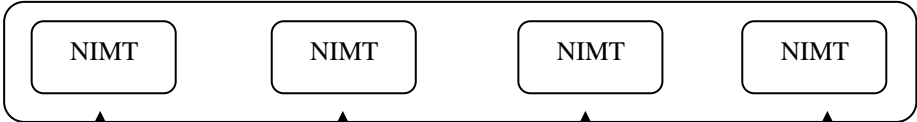

Working Standard
Calibration Laboratory

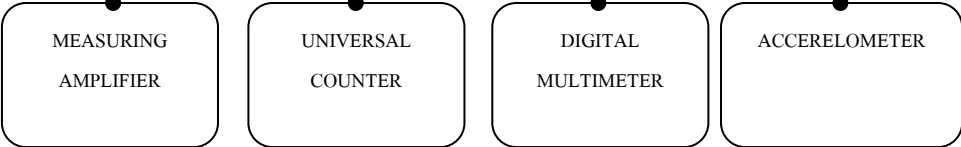

MEASURING AMPLIFIER
BRUEL&KJAER MODEL 2525 ACCURACY ±0.01%

UNIVERSAL COUNTER
HP MODEL 5315A ACCURACY ± 0.01%

DIGITAL MULTIMETER
HP MODEL 34401A ACCURACY ± 0.06%

ACCERELOMETER
BRUEL&KJAER MODEL 8305
ACCURACY ± 0.05%

Vibration Instrument

